

## COMPARISON OF THE EMPIRICAL VARIANCES AND MEAN VALUES OF NORMALLY DISTRIBUTED POPULATIONS OF NUCLEAR COUNTS

by

**Djordje R. LAZAREVIĆ<sup>1\*</sup>, Marija D. OBRENOVIĆ<sup>2</sup>,  
Irfan S. FETAHOVIĆ<sup>3</sup>, and Predrag V. OSMOKROVIĆ<sup>2</sup>**

<sup>1</sup>Vinča Institute of Nuclear Sciences, University of Belgrade, Belgrade, Serbia

<sup>2</sup>Faculty of Electrical Engineering, University of Belgrade, Belgrade, Serbia

<sup>3</sup>State University of Novi Pazar, Novi Pazar, Serbia

Scientific paper

DOI: 10.2298/NTRP1404285L

This paper discusses the possibility of applying the F-test and double t-test in problems related to the identification of number of radioactive isotopes in a contaminated area by using only counters for radiation detection. The descriptions of the F-test and the double t-test are given along with the corresponding tabular values that enable their implementation. Finally, the experiment is presented via two radioactive samples. The results of the experiment were treated in the manner proposed in the paper and satisfactory results were obtained.

*Key words: nuclear count, F-test, double t-test, variance*

### INTRODUCTION

The development of mathematical algorithms, no matter how complex they might look, enables us to quickly adopt adequate conclusions on a statistical behavior of random variable. Since the environment is increasingly contaminated by electromagnetic and particle radiation, one of the most important tasks, in the field of radiation protection, is to identify the sources of radiation.

This implies radiation detection and the determination of the source of radiation. It is particularly important to determine the number of radiation sources and separate the effects of irradiation related to the particular source in a contaminated area. This is of particular interest for the proper functioning of electronic systems in areas exposed to radiation [1-3].

The field of radiation protection often involves the detection of nuclear radiation in contaminated environments. Such measurements are used to determine whether there is a radioactive source (one or more) in order to eliminate its effect in the process of decontamination. However, in practice, the investigated area is frequently contaminated with several radioactive sources [4, 5].

For this reason, it is useful to develop a mathematical method that can determine whether the de-

tected radiation comes from one or several sources. The aim of this paper is to develop an algorithm for establishing two or more normally distributed populations of nuclear counting results that originate from one or more of the radioactive sources by using only radiation counter as a detector [6, 7].

### COMPARISON OF EMPIRICAL VARIANCE AND MEAN VALUES

To determine if two normally distributed populations originate from a radioactive source involves proving the statistical equality of their variances and mean values. An F-test is used for the comparison of variances and a double t-test for the comparison of mean values.

The basis of the F-test is F-distribution, defined in the following way: if  $y$  and  $z$  are independent variables that have  $\chi_2$  distribution with degrees of freedom  $m_1$  and  $m_2$ , the ratio  $X = (y/m_1)/(z/m_2)$  is the F-distribution with degrees of freedom  $m_1$  and  $m_2$ . Its probability density function is described as following

$$f_F(x) = \frac{1}{B\left(\frac{m_1}{2}, \frac{m_2}{2}\right)} \frac{\left(\frac{m_1}{2}\right)^{\frac{m_1}{2}} x^{\frac{m_1}{2}-1} \left(\frac{m_2}{2}\right)^{\frac{m_2}{2}}}{\left(\frac{m_1}{2} + \frac{m_2}{2} x\right)^{\frac{m_1+m_2}{2}}}, \quad x > 0 \quad (1)$$

\* Corresponding author; e-mail: djordje.lazarevic@vinca.rs

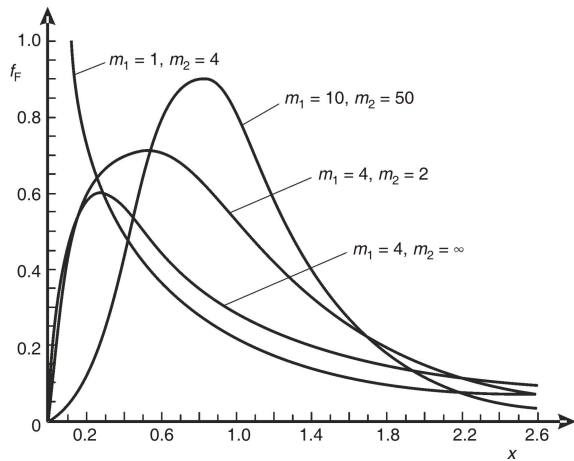


Figure 1. Probability density function characteristic  $f_F(x)$  of F distribution with  $m_1$  and  $m_2$  degrees of freedom as parameters

Table 1. Quantiles  $q$  of F-distribution  $F_{m_1:m_2;q}$

$m_2$	$m_1$					
	6	8	10	13	16	20
(a) $q = 0.95$						
6	4.28	4.15	4.06	3.98	3.92	3.87
8	3.58	3.44	3.35	3.26	3.20	3.15
10	3.22	3.07	2.98	2.89	2.83	2.77
13	2.92	2.77	2.67	2.58	2.51	2.46
16	2.74	2.59	2.49	2.40	2.33	2.28
20	2.60	2.45	2.35	2.25	2.18	2.12
(b) $q = 0.975$						
6	5.82	5.60	5.46	5.33	5.24	5.17
8	4.65	4.43	4.30	4.16	4.08	4.00
10	4.07	3.85	3.72	3.58	3.50	3.42
13	3.60	3.39	3.25	3.11	3.03	2.95
16	3.34	3.12	2.99	2.85	2.76	2.68
20	3.13	2.91	2.77	2.64	2.55	2.46

where  $B(r,s) = \int_0^1 x^{r-1} (1-x)^{s-1} dx$  represents a Beta function.

The probability density function characteristic is given in fig. 1 with  $m_1$  and  $m_2$  degrees of freedom as parameters. Table 1 shows quantiles  $q$  of F-distribution  $F_{m_1:m_2;q}$  [8, 9].

The basis of the double t-test is t-distribution, which is defined in the following way: if  $y$  and  $z$  are independent random variables, and if  $y$  has a normal distribution  $N(0; 1)$ , and if  $z$  has a  $\chi^2$  distribution with  $m$  degrees of freedom, the quotient  $x = y/(2/m)^{1/2}$  has a t-distribution with  $m$  degrees of freedom. In addition, the quotient of the two independent variables having a normal  $N(0; 1)$  distribution has a t-distribution with  $m = 1$  degrees of freedom. The probability density function of the t-distribution is

$$f_1(x) = \frac{\Gamma\left(\frac{m+1}{2}\right) \left(1 + \frac{x^2}{m}\right)^{-\frac{m+1}{2}}}{\Gamma\left(\frac{m}{2}\right) \sqrt{\pi m}} \quad (2)$$

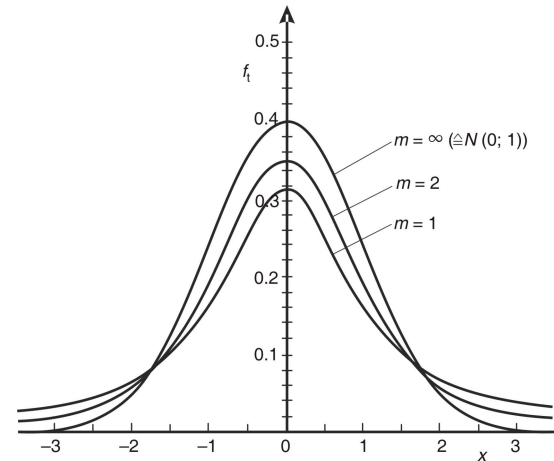


Figure 2. Probability density function  $f_t(x)$  of t-distribution with degrees of freedom  $m$  as parameter

Table 2. t-distribution quantiles  $t_{m;q}$

$m$	Quantiles $t_{m;q}$		
	$q = 0.95$	$q = 0.975$	$q = 0.99$
1	6.31	12.7	31.8
2	2.92	4.30	6.96
3	2.35	3.18	4.54
4	2.13	2.78	3.75
5	2.02	2.57	3.37
7	1.89	2.36	3.00
9	1.83	2.26	2.82
14	1.76	2.14	2.62
19	1.73	2.09	2.54
24	1.71	2.06	2.49
40	1.68	2.02	2.42
120	1.66	1.98	2.36
$\infty$	1.64	1.96	2.33

The probability density function of the t-distribution is shown in fig. 2. Quantiles  $t_{m;q}$  of t-distribution are given in tab. 2.

The comparison of the two empirical variances in the F-test is performed on the basis of the following hypotheses: the variance of two normally distributed populations  $\sigma_x^2$  and  $\sigma_y^2$  represented by the size of two samples  $u_x$  and  $u_y$ ; the empirical  $s_x^2$  and  $s_y^2$  variances are equal if  $\sigma_x^2 = \sigma_y^2$ . To test the hypothesis the size taken is

$$t = \frac{s_x^2}{s_y^2} \quad (3)$$

where  $x$  and  $y$  have to be chosen so that  $s_x^2 = s_y^2$ .

The critical value of  $F_{m_1:m_2;q}$  is based on tab. 1, from the F distribution, as a quantile with a degree of freedom  $m_1 = n_x - 1$  and  $m_2 = n_y - 1$ , and an order of  $q = 1 - \alpha/2$  (double t-test at  $\alpha$  level of significance). The hypothesis is discarded if  $t > F_{m_1:m_2;q}$ .

The comparison of the mean values, by using the two double t-tests, is based on the following hypotheses.

The two mean values  $\mu_x$  and  $\mu_y$ , normally distributed with a population of the equal variance (assuming a double t-test does not discard the F-test), which can assume a size of the two samples  $n_x$  and  $n_y$ , the mean values  $\bar{x}$  and  $\bar{y}$ , and empirical variances  $s_x^2$  and  $s_y^2$ , are equal to  $\mu_x = \mu_y$ .

To test the hypothesis, the size taken is

$$t = \frac{(\bar{x} - \bar{y}) \sqrt{\frac{n_x n_y}{n_x + n_y}}}{\sqrt{\frac{(n_x - 1)s_x^2 + (n_y - 1)s_y^2}{n_x + n_y - 2}}} \quad (4)$$

The critical value of  $t_{m,q}$  is obtained on the basis of tab. 2, degree of freedom  $m = n_x + n_y - 2$  and order  $q = 1 - \alpha/2$  (two-sided test at  $\alpha$  significance level). The hypothesis is rejected if  $|t| > t_{m,q}$  [10, 11].

## EXPERIMENT

A radioactive source was placed in the laboratory ( $^{137}\text{Cs}$ ). After that, 21 pulse measurements with the GM counter were performed at intervals of 5 minutes. The procedure was then repeated, with the exception that, in the laboratory, another source of radiation was added ( $^{241}\text{Am}$ ) [12, 13].

## RESULTS AND DISCUSSION

At first, two measurements of empirical variances  $s_1 = 64,4$  and  $s_2 = 57,8$  of two normally distributed populations were obtained. Since  $s_1 > s_2$  then  $s_1^2 = s_x^2, s_2^2 = s_y^2, n_1 = n_x, n_2 = n_y$ . On the basis of expression (3), the test statistic  $t = 1.24$  is obtained. The hypothesis has been tested at a significance level  $\alpha = 0.05$  ( $q = 0.975$ ) with  $m_1 = m_2 = 20$ . From tab. 1, a critical value  $F_{20;20;0.975}$  was obtained. Having that  $1.24 < 2.46$ , the hypothesis that these two samples were obtained from populations with the same variance cannot be rejected.

As already mentioned, there was no rejection of the hypothesis on the basis of the F-test that was performed. The hypothesis of equality of the mean values was then validated by the double t-test. On the basis of expression (4) and the fact that the mean values are 2980 and 3032, and that the variance can be considered the same, a test statistic that equals 1.12 was obtained, while critical value  $t_{40;0.975} = 2.02$  is taken from tab. 2.

Considering that  $1.12 < 2.02$ , the hypothesis cannot be rejected. The samples are therefore obtained from the population distributed in the same manner.

Further, the measurements of two samples with two radiation source included were taken. Through measurements of two samples, variances  $s_1 = 130.37$  and  $s_2 = 68.9$

were obtained with the mean values being 3120 and 2310. Since  $s_1 > s_2$  then  $s_1^2 = s_x^2, s_2^2 = s_y^2, n_1 = n_x$ , and  $n_2 = n_y$ . On the basis of expression (3), a test statistic  $t = 3.58$  is obtained. If the hypothesis is tested at a significance level of with  $m_1 = m_2 = 20$ , from tab. 1 the critical value  $F_{20;20;0.975} = 2.46$  is obtained. Since,  $3.58 > 2.46$ , the hypothesis that these two samples were obtained from the same population can be rejected.

## CONCLUSION

The proposed method of applying the F-test and double t-test provides a simple experimental procedure and an even simpler method of mathematical statistics as a basis for determining the number and type (under certain conditions) of radioactive isotopes that have contaminated a facility or an area.

The proposed method could, in addition to these applications, find use in other, similar areas of dosimetry and radiation protection.

## ACKNOWLEDGEMENTS

The Ministry of Education, Science and Technological Development of the Republic of Serbia supported this work under contract 171007.

## AUTHOR CONTRIBUTIONS

Theoretical analysis carried out by Dj. R. Lazarević and M. D. Obrenović. Simulations and calculations were carried out by Dj. R. Lazarević and I. S. Fetahović. All authors analyzed and discussed the results. The manuscript was written by Dj. R. Lazarević and M. D. Obrenović, and the figures and tables were prepared by Dj. R. Lazarević.

## REFERENCES

- [1] Marjanović, N., et al., Effects of Heavy Ion Bombardment on  $\text{TiO}_2$  Memristor Operation, *Radiation Effects and Defects in Solids*, 166 (2011), 1, pp. 1-7
- [2] Dolićanin, Č. B., et al., Statistical Treatment of Nuclear Counting Results, *Nucl Technol Radiat.*, 26 (2011), 2, pp. 164-170
- [3] Cavrić, B., et al., Radiation Hardness of Flash Memory Fabricated in Deep-Submicron Technology, *International Journal of Photoenergy*, Vol. 2013, 2013, Article number 158792
- [4] Holmes-Siedle, A. Adams, L., Handbook of Radiation Effects, Oxford Science Publication, Oxford, UK, 1993
- [5] Pejović, M. M., et al., Experimental Investigation of Breakdown Voltage and Electrical Breakdown Time Delay of Commercial Gas Discharge Tubes, *Nucl Technol Radiat*, 27 (2012), 4, pp. 341-345
- [6] Dolićanin, D., Pučić D., Stanković, K., Application of mixed Multiplicative Statistical Distributions in De-

- signing Vacuum Insulation Systems, *Vacuum*, 100 (2014), pp. 7-10
- [7] Hauschild, W., Mosch, W., Statistical Techniques for High voltage, English edition, Peter Peregrinus Ltd, London, 1992
- [8] Osmokrović, P., et al., Determination of Pulse Tolerable Voltage in Gas-Insulated Systems, *Japanese Journal of Applied Physics*, 47(2008), 12, pp. 8928-8934
- [9] Dekić, S., et al., Conditions for the Applicability of the Geometrical Similarity Law to Impulse Breakdown in Gases, *IEEE Transactions on Dielectrics and Electrical Insulation*, 17 (2010), 4, pp. 1185-1195, Article number 5539689
- [10] Stanković, S. J., et al., MSV Signal Processing System for Neutron-Gamma Discrimination in a Mixed Field, *Nucl Technol Radiat*, 27(2012), 2, pp. 165-170
- [11] Stanković, K., et al., Statistical Analysis of the Characteristics of Some Basic Mass-Produced Passive Electrical Circuits Used in Measurements, *Measurement: Journal of the International Measurement Confederation*, 44 (2011), 9, pp. 1713-1722
- [12] Vujisić, M., et al., Radiation Hardness of COTS EPROMs and EEPROMs, *Radiation Effects and Defects in Solids: Incorporating Plasma Science and Plasma Technology*, 165 (2010), 5, pp. 362-369
- [13] Stanković, K., Osmokrović, P., The model for Calculating the Type a Measurement Uncertainty of GM Counters from the Aspect of Device Miniaturization, *IEEE Transactions on Nuclear Science*, 61 (2014), 3, pp. 1316-1325, Article number 6819052
- [14] Stanković, K. D. , Influence of the Plain-Parallel Electrode Surface Dimensions on the Type a Measurement Uncertainty of gm Counter, *Nucl Technol Radiat*, 26 (2011), 1, pp. 39-44

Received on September 12, 2014

Accepted on November 29, 2014

**Ђорђе Р. ЛАЗАРЕВИЋ, Марија Д. ОБРЕНОВИЋ,  
Ирфан С. ФЕТАХОВИЋ, Предраг В. ОСМОКРОВИЋ**

**ПОРЕЂЕЊЕ ДОБИЈЕНЕ ЕМПИРИЈСКЕ ВАРИЈАНСЕ И СРЕДЊИХ ВРЕДНОСТИ  
НОРМАЛНО РАСПОДЕЉЕНИХ ПОПУЛАЦИЈА НУКЛЕАРНОГ ОДБРОЈА**

У раду се разматра могућност примене F-теста и t-дуплог теста у проблемима везаним за идентификацију броја радиоактивних изотопа, који се налазе у контаминираним подручјима, када се за детекцију зрачења користе бројачи. Описи F-теста и t-дуплог теста су дати заједно са одговарајућим табеларним вредностима које омогућавају њихово спровођење. Експеримент је спроведен са два радиоактивна извора. Резултати експеримента су третирани на начин предложен у самом раду при чему су добијени задовољавајући резултати.

*Кључне речи:* нуклеарни одброј, F-тест, t-дупли тест, варијанса